



Total Quality. Assured.

TEST REPORT



中国认可
国际互认
检测
TESTING
CNAS L0220

Number: GZHT90984373

Date: Aug 14, 2020

Applicant: HONEYWELL SALISBURY
4091 AZALEA DRIVE, NORTH CHARLESTON,
USA

Attn: RAMESH KANNAN

Sample Description:

- Three (3) groups of submitted samples said to be:
- (A) Twelve (12) pairs 52000 Men's safety boots in Red/Black
- (B) Twelve (12) pairs 52001 Men's safety boots in Red/Black
- (C) Five (5) pairs of Non-metallic insole boards used for Sample B.

Test Standard/Method : CSA Z195-14
ASTM F2413-18
ASTM F2913-19
SATRA TM144: 2011

Size : 6, 9, 12, 16

Buyer's Name : --

Ref. No : 52000 & 52001

Brand : --

Manufacturer : --

Colour : Red/Black

Vendor : --

Supplier : --

P.O. No. : 178358

Toe Cap : Non Metallic

Vamp Lining : CR

Quarter Lining : XR

Seat Region Lining : CR

Sole : Rubber

Country Of Origin : China

Goods Exported To : U.S.A.

Date Received/Date Test Started : Aug. 06, 2020

Date Final Information Confirmed: --

Test Result Please Refer To Attached Page(S).

Should you have any query on this report, you may contact at gzfootwear@intertek.com

Authorized By:
For Intertek Testing Services Shenzhen Ltd.
Guangzhou Branch



Guiliang Dong
Senior Lab Manager



MI / bettyxlchen

Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

深圳天祥质量技术服务有限公司广州分公司

Room 02, 1-8/F. & Room 01, E101/E201/E301/E401/E501/E601/E701/E801,
No.7-2, Caipin Road, Guangzhou Science City, GETDD, Guangzhou, Guangdong, China
广州经济技术开发区科学城彩频路7号之二第1-8层02房、01房101、
E201、E301、E401、E501、E601、E701、E801
Tel: +86 208213 9001 Fax: +86 20 82089909 Postcode: 510663

3/F., Hengyun Building, 235 Kaifa Ave., Guangzhou
Economic & Technological Development District, Guangzhou,
China
中国广州经济技术开发区开发大道235号恒运大厦3楼
Tel: +86 20 83966868 Fax: +86 20 82228169 Postcode: 510730



1 Protective Toe Impact Resistance (I) (ASTM F2412-18a, 5, Impact Force: 101.7 J (75 lbf), Testing Performed At 22 °C And 50% RH)

	(A)	<u>ASTM F2413-18 Requirement</u>	<u>Pass / Fail</u>
	Interior Height Clearance		
Left:	25.5 mm	≥ 12.7 mm	Pass
Right:	27.4 mm	≥ 12.7 mm	Pass
Left:	27.2 mm	≥ 12.7 mm	Pass

	(B)	<u>ASTM F2413-18 Requirement</u>	<u>Pass / Fail</u>
	Interior Height Clearance		
Left:	22.8 mm	≥ 12.7 mm	Pass
Right:	24.9 mm	≥ 12.7 mm	Pass
Left:	24.3 mm	≥ 12.7 mm	Pass

2 Protective Toe Compression Resistance (C) (ASTM F2412-18a, 6, Compression Force: 11 121 N (2 500 lbf), Testing Performed At 22 °C And 50% RH)

	(A)	<u>ASTM F2413-18 Requirement</u>	<u>Pass/Fail</u>
	Interior Height Clearance		
Left:	23.1 mm	≥ 12.7 mm	Pass
Right:	26.0 mm	≥ 12.7 mm	Pass
Right:	24.0 mm	≥ 12.7 mm	Pass

	(B)	<u>ASTM F2413-18 Requirement</u>	<u>Pass/Fail</u>
	Interior Height Clearance		
Left:	23.0 mm	≥ 12.7 mm	Pass
Right:	21.2 mm	≥ 12.7 mm	Pass
Right:	22.8 mm	≥ 12.7 mm	Pass



3 Puncture Resistance Footwear (PR) (ASTM F2412-18a, 11, Conditioned At 22 °C And 50 % RH For 24 h And Testing Performed At The Same Conditions.)

	(C)	<u>ASTM F2413-18 Requirement</u>	<u>Pass/Fail</u>
Left:	The Test Pin Did Not Penetrate Beyond The Face Of The Material Nearest The Foot Before 1 200 N.	Min. 1 200 N (*)	Pass
Right:	The Test Pin Did Not Penetrate Beyond The Face Of The Material Nearest The Foot Before 1 200 N.	Min. 1 200 N (*)	Pass
Right:	The Test Pin Did Not Penetrate Beyond The Face Of The Material Nearest The Foot Before 1 200 N.	Min. 1 200 N (*)	Pass

Remark: * = The Test Pin Does Not Visually Penetrate Beyond The Face Of The Material Nearest The Foot.

4 Flex Resistance For Puncture Resistant Devices (ASTM F2412-18a, 11.7 & CSA Z195-14, 6.3.2)

	(C)	<u>ASTM F2413-18 Requirement</u>	<u>Pass/Fail</u>
Left:	No Signs Of De-lamination Of Layers Or Cracking After 1.5 x 10 ⁶ Flexes.	*	Pass
Right:	No Signs Of De-lamination Of Layers Or Cracking After 1.5 x 10 ⁶ Flexes.	*	Pass
Left:	No Signs Of De-lamination Of Layers Or Cracking After 1.5 x 10 ⁶ Flexes.	*	Pass

Remark: * = No Signs Of De-lamination Of Layers Or Cracking After 1.5 x 10⁶ Flexes.



5 Toecap Impact Resistance (CSA Z195-14, 6.2, Grade 1: 125 Joules)

(A)		The Internal Toe Clearance	Requirement	Pass/Fail
Size M's 9	Left:	23.2 mm	Min. 12.7 mm (*)	Pass
	Right:	24.1 mm	Min. 12.7 mm (*)	Pass
(B)		The Internal Toe Clearance	Requirement	Pass/Fail
Size M's 9	Left:	21.8 mm	Min. 12.7 mm (*)	Pass
	Right:	22.0 mm	Min. 12.7 mm (*)	Pass

Remark: * = In Addition, The Protective Toecap Shall Not Fracture Through Its Thickness.

6 Toecap Impact Resistance (CSA Z195-14, 5.1.1, -18 °C x 12h Grade 1: 125 Joules)

(A)		The Internal Toe Clearance	Requirement	Pass/Fail
Size M's 9	Left:	26.2 mm	Min. 12.7 mm (*)	Pass
	Right:	27.2 mm	Min. 12.7 mm (*)	Pass
(B)		The Internal Toe Clearance	Requirement	Pass/Fail
Size M's 9	Left:	25.2 mm	Min. 12.7 mm (*)	Pass
	Right:	25.4 mm	Min. 12.7 mm (*)	Pass

Remark: * = In Addition, The Protective Toecap Shall Not Fracture Through Its Thickness.

7 Slip Resistance(ASTM F2913-19)

Conditioning For Specimen:

Temperature: (23±2) °C
Relative Humidity: (50±5)%
Period: At Least 3 Hours

Test Condition:

Test Surface: Clay Tile
Vertical Force: 500 N

Sample	Size	Sequence	Conditions	Modes	Results
(A)	9 (Left)	Wet After Dry	Dry	Forward Heel Slip	0.84
				Backward Forepart Slip	1.38
				Forward Flat Slip	1.24
			Wet	Forward Heel Slip	0.74
				Backward Forepart Slip	0.78
				Forward Flat Slip	0.84
	(Right)	Dry After Wet	Wet	Forward Heel Slip	0.73
				Backward Forepart Slip	0.80
			Dry	Forward Flat Slip	0.82
				Forward Heel Slip	0.85
			Backward Forepart Slip	1.33	
			Forward Flat Slip	1.20	

Sample	Size	Sequence	Conditions	Modes	Results
(B)	9 (Left)	Wet After Dry	Dry	Forward Heel Slip	0.85
				Backward Forepart Slip	0.84
				Forward Flat Slip	0.98
			Wet	Forward Heel Slip	0.55
				Backward Forepart Slip	0.58
				Forward Flat Slip	0.57
	(Right)	Dry After Wet	Wet	Forward Heel Slip	0.54
				Backward Forepart Slip	0.58
				Forward Flat Slip	0.60
			Dry	Forward Heel Slip	0.88
				Backward Forepart Slip	0.85
				Forward Flat Slip	0.99

Note:

It Must Be Noted That The Slip Resistance Test Carried Out In This Report Denotes An Indication Of Slip Of This Particular Footwear/Component On The Surface Mentioned In The Test Item. It Is Important To Note That Footwear Is Subject To Many Different Conditions Encountered In Everyday Use And That It Is Impossible To Make Footwear Resistant To Slip In All Conditions. Nevertheless, It Is Generally Accepted That Problems Are Minimized If The Guideline Coefficients Of Friction Are Achieved.



8 Slip Resistance (SATRA TM144: 2011, Ice Surface At -7°C, Vertical Force: 500 N)


(B)

	Dry Smooth Icy	Wet Icy
Heelpart	0.20	0.15
Forepart	0.14	0.09
Heelpart	0.23	0.16
Forepart	0.16	0.10

Note:

1. The Outsole Of Test Sample Was Pre-Chilled To -7°C In Water-Ethanol Bath Before Testing.
2. It Must Be Noted That The Slip Resistance Test Carried Out In This Report Denotes An Indication Of Slip Of This Particular Footwear/Component On The Surface Mentioned In The Test Item. It Is Important To Note That Footwear Is Subject To Many Different Conditions Encountered In Everyday Use And That It Is Impossible To Make Footwear Resistant To Slip In All Conditions. Nevertheless, It Is Generally Accepted That Problems Are Minimized If The Guideline Coefficients Of Friction Are Achieved.

Expended Uncertainty: 0.01, With k = 2 At 95% Confidence Level.

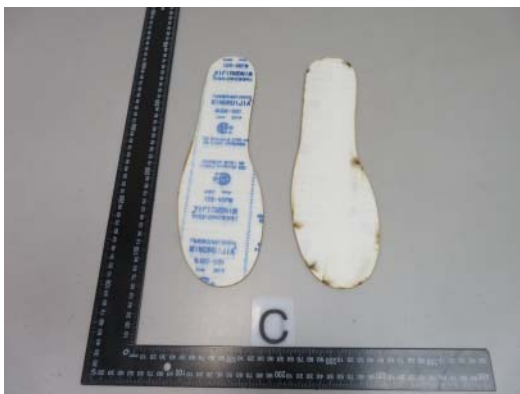

End Of Report

This report is made solely on the basis of your instructions and/or information and materials supplied by you. It is not intended to be a recommendation for any particular course of action. Intertek does not accept a duty of care or any other responsibility to any person other than the Client in respect of this report and only accepts liability to the Client insofar as is expressly contained in the terms and conditions governing Intertek's provision of services to you. Intertek makes no warranties or representations either express or implied with respect to this report save as provided for in those terms and conditions. We have aimed to conduct the Review on a diligent and careful basis and we do not accept any liability to you for any loss arising out of or in connection with this report, in contract, tort, by statute or otherwise, except in the event of our gross negligence or wilful misconduct. No copy of the test report(except for full text copy) shall be made without the written approval by Intertek.