

Product Data Sheet

Product Datasheet

H2S 3E 2000 S Hydrogen Sulfide Gas Sensor

Document Purpose

The purpose of this document is to present the performance specification of the H2S 3E 2000 S hydrogen sulfide gas sensor.

This document should be used in conjunction with Operating Principles (OP08).

The data provided in this document are valid at 20°C, 50% RH and 1013 mBar for 3 months from the date of sensor manufacture.

Output signal can drift below the lower limit over time. For guidance on the safe use of the sensor, please refer to the Operating Principles OP08.

Product Data Sheet

- Key Features & Benefits:**
- High range H₂S sensor
 - High capacity
 - Very Selective

Technical Specifications

MEASUREMENT

| | |
|-------------------------------------|--|
| Operating Principle | 3-electrode electrochemical |
| Measurement Range | 0-2000 ppm H ₂ S |
| Lower Detection Limit | <20 ppm |
| Filter | None |
| Sensitivity* | 60 ± 25 nA/ppm |
| Response Time (T90)* | < 60 s <small>calculated from 2 minute exposure time</small> |
| Baseline Offset (clean air)* | < ±250 nA |

ELECTRICAL

| | |
|----------------------------------|---|
| Recommended Load Resistor | 10 Ω |
| Bias Voltage | 0 mV |
| Resolution | Dependent on Electronics : < 7 ppm when using recommended circuitry |

MECHANICAL

| | |
|--------------------------------|--|
| Housing Material | ABS |
| Weight | 2.4 g : Mini 4.7 g : 4-Series 7.0 g : 7-Series 2.9 g : Smart 3.4 g : Classic |
| Recommended Orientation | Membrane / filter pointing downwards or horizontal direction |

ENVIRONMENTAL

| | |
|------------------------------------|------------------------------|
| Typical Applications | Biogas, Landfill |
| Operating Temperature Range | -20°C to +50°C |
| Operating Pressure Range | Atmospheric ± 10% |
| Operating Humidity Range | 15% to 90% RH non-condensing |


INTRINSIC SAFETY DATA

| | |
|----------------------------|--------|
| Maximum at 2000ppm | 170 mA |
| Maximum o/c Voltage | 500 mV |
| Maximum s/c Current | 500 µA |

LIFETIME

| | |
|--------------------------------|-----------------------------|
| Long Term Output Drift* | < 15% per 6 months |
| Expected Operating Life | >15 months in normal use |
| Storage Life | 8 weeks in sealed container |

Available in:

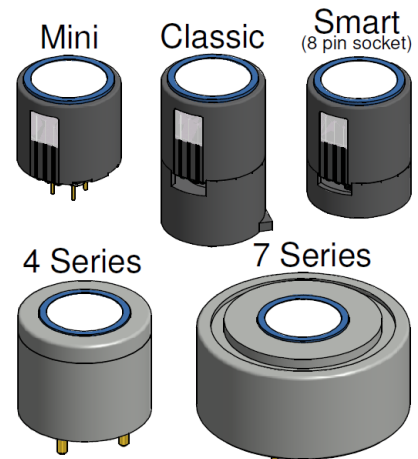

IMPORTANT NOTE: Connection should be made via PCB sockets only. Soldering to pins will render your warranty void.

Part Numbers

| H2S 3E 2000 S | Part Number |
|---------------|-------------------|
| Mini | 75-0155-134-30009 |
| Classic | 75-0155-134-30069 |
| Smart | 75-0155-134-32259 |
| 4-Series | 75-0155-134-30049 |
| 7-Series | 75-0155-134-30079 |


Orders should be placed through Sensoric Gas Sensors in Bonn.

For the H2S 3E 2000 S Transmitter with 4-20 mA output, refer to the H2S 3E 2000 S Transmitter datasheet

* Specifications are valid at 20°C, 50% RH and 1013 mBar, using recommended circuitry. Performance characteristics outline the performance of sensors supplied within the first 3 months. Output signal can drift below the lower limit over time.

Product Data Sheet

Product Dimensions

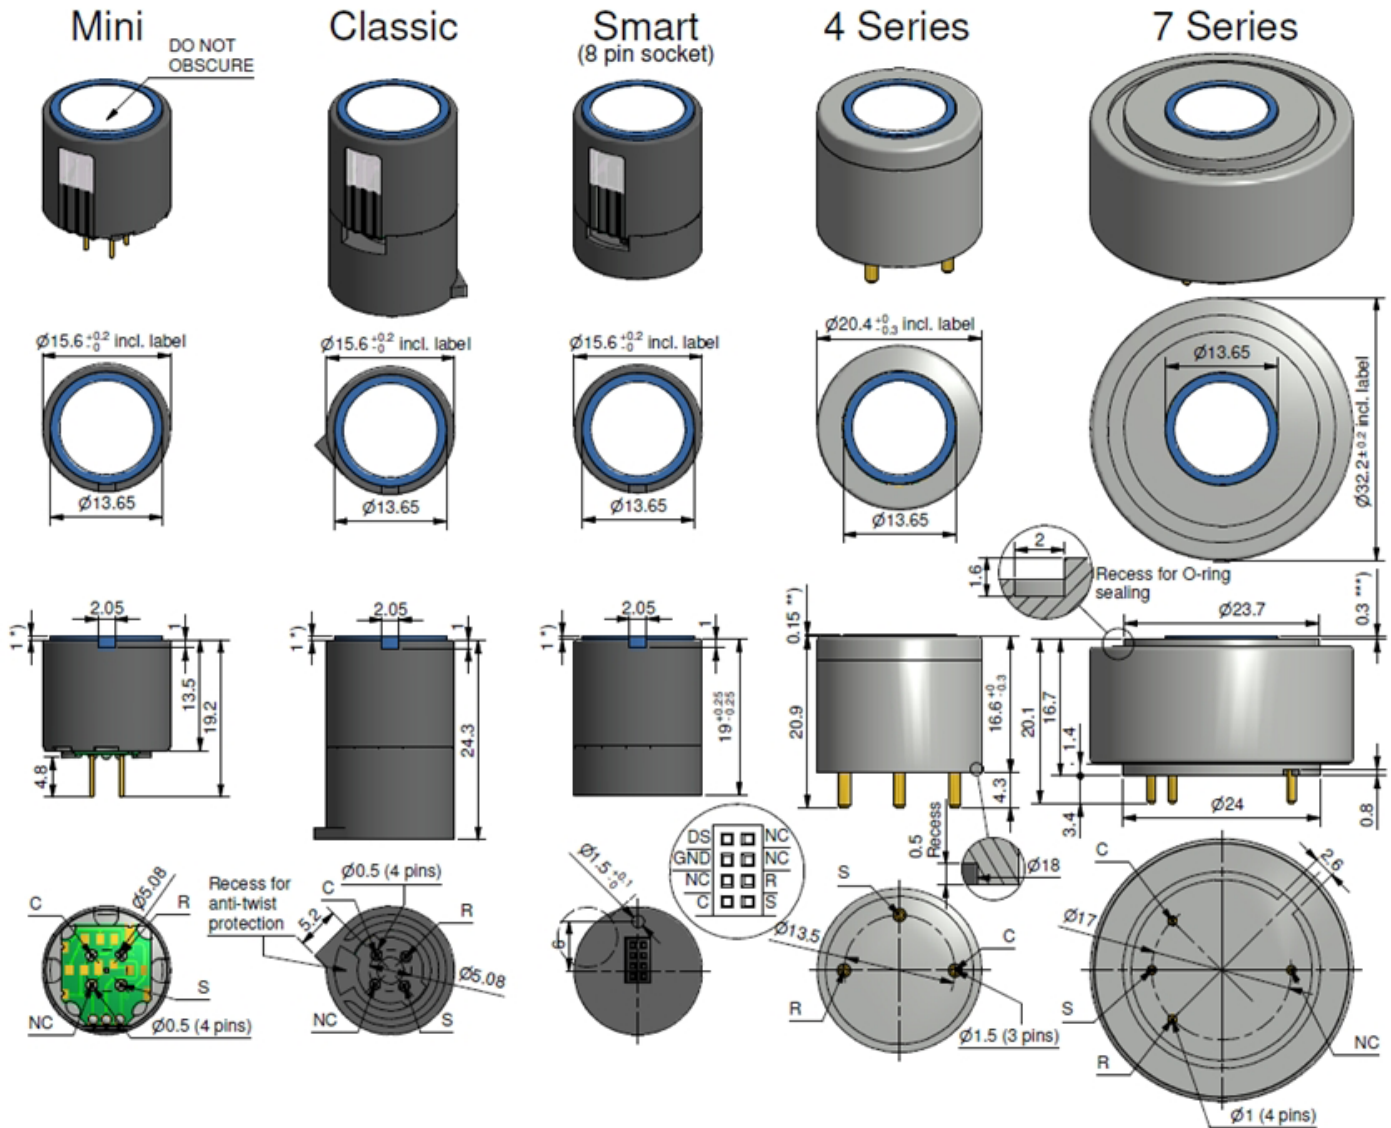

All dimensions in mm
All tolerances ± 0.15 mm unless otherwise stated

S Sensing
C Counter
R Reference
NC Not Connected

*) Projection 0.6 - 1.25 mm depending on gastype
**) Projection up to 0.4 mm for 4 Series
***) Projection up to 0.55 mm for 7 Series
Please contact sales_europe@citytech.com for details information

Important Note: Connection should be made via PCB sockets only. Soldering to the pins will void the warranty.

Plugs and customised adaptations available on request

This drawing may be subject to corrections or changes without prior notice

© LSD AG - COMMERCIAL IN CONFIDENCE - NOT TO BE REPRODUCED WITHOUT CONSENT

Product Data Sheet

Poisoning

Sensoric cells are designed for operation in a wide range of environments and harsh conditions. However, it is important that exposure to high concentrations of solvent vapours is avoided, both during storage, fitting into instruments, and operation.

When using sensors with printed circuit boards (PCBs), degreasing agents should be used before the sensor is fitted. Do not glue directly on or near the Sensoric cells as the solvent may cause crazing of the plastic.

Cross Sensitivity Table

Whilst sensors are designed to be highly specific to the gas they are intended to measure, they will still respond to some degree to various other gases. The table below is not exclusive and other gases not included in the table may still cause a sensor to react.

IMPORTANT NOTE : The cross sensitivity data shown below does not form part of the product specification and is supplied for guidance only. Values quoted are based on tests conducted on a small number of sensors and any batch may show significant variation. For the most accurate measurements, an instrument should be calibrated using the gas under investigation.

| Gas | Concentration Used | Reading (ppm H ₂ S) |
|--|--------------------|--------------------------------|
| Ammonia, NH ₃ | 1000 ppm | 0 |
| Carbon Dioxide, CO ₂ | 50% | 0 |
| Hydrogen, H ₂ | 2% | <110 |
| Iso Propyl Alcohol, C ₃ H ₇ OH | 8900 ppm | 0 |
| Methane, CH ₄ | 60% | 0 |

SAFETY NOTE

This sensor is designed to be used in safety critical applications. To ensure that the sensor and/or instrument in which it is used, are operating properly, it is a requirement that the function of the device is confirmed by exposure to target gas (bump check) before each use of the sensor and/or instrument. Failure to carry out such tests may jeopardize the safety of people and property.

Every effort has been made to ensure the accuracy of this document at the time of printing. In accordance with the company's policy of continued product improvement City Technology Limited reserves the right to make product changes without notice. The products are always subject to a programme of improvement and testing which may result in some changes in the characteristics quoted. As the products may be used by the client in circumstances beyond the knowledge and control of City Technology Limited, we cannot give any warranty as to the relevance of these particulars to an application. It is the clients' responsibility to carry out the necessary tests to determine the usefulness of the products and to ensure their safety of operation in a particular application.